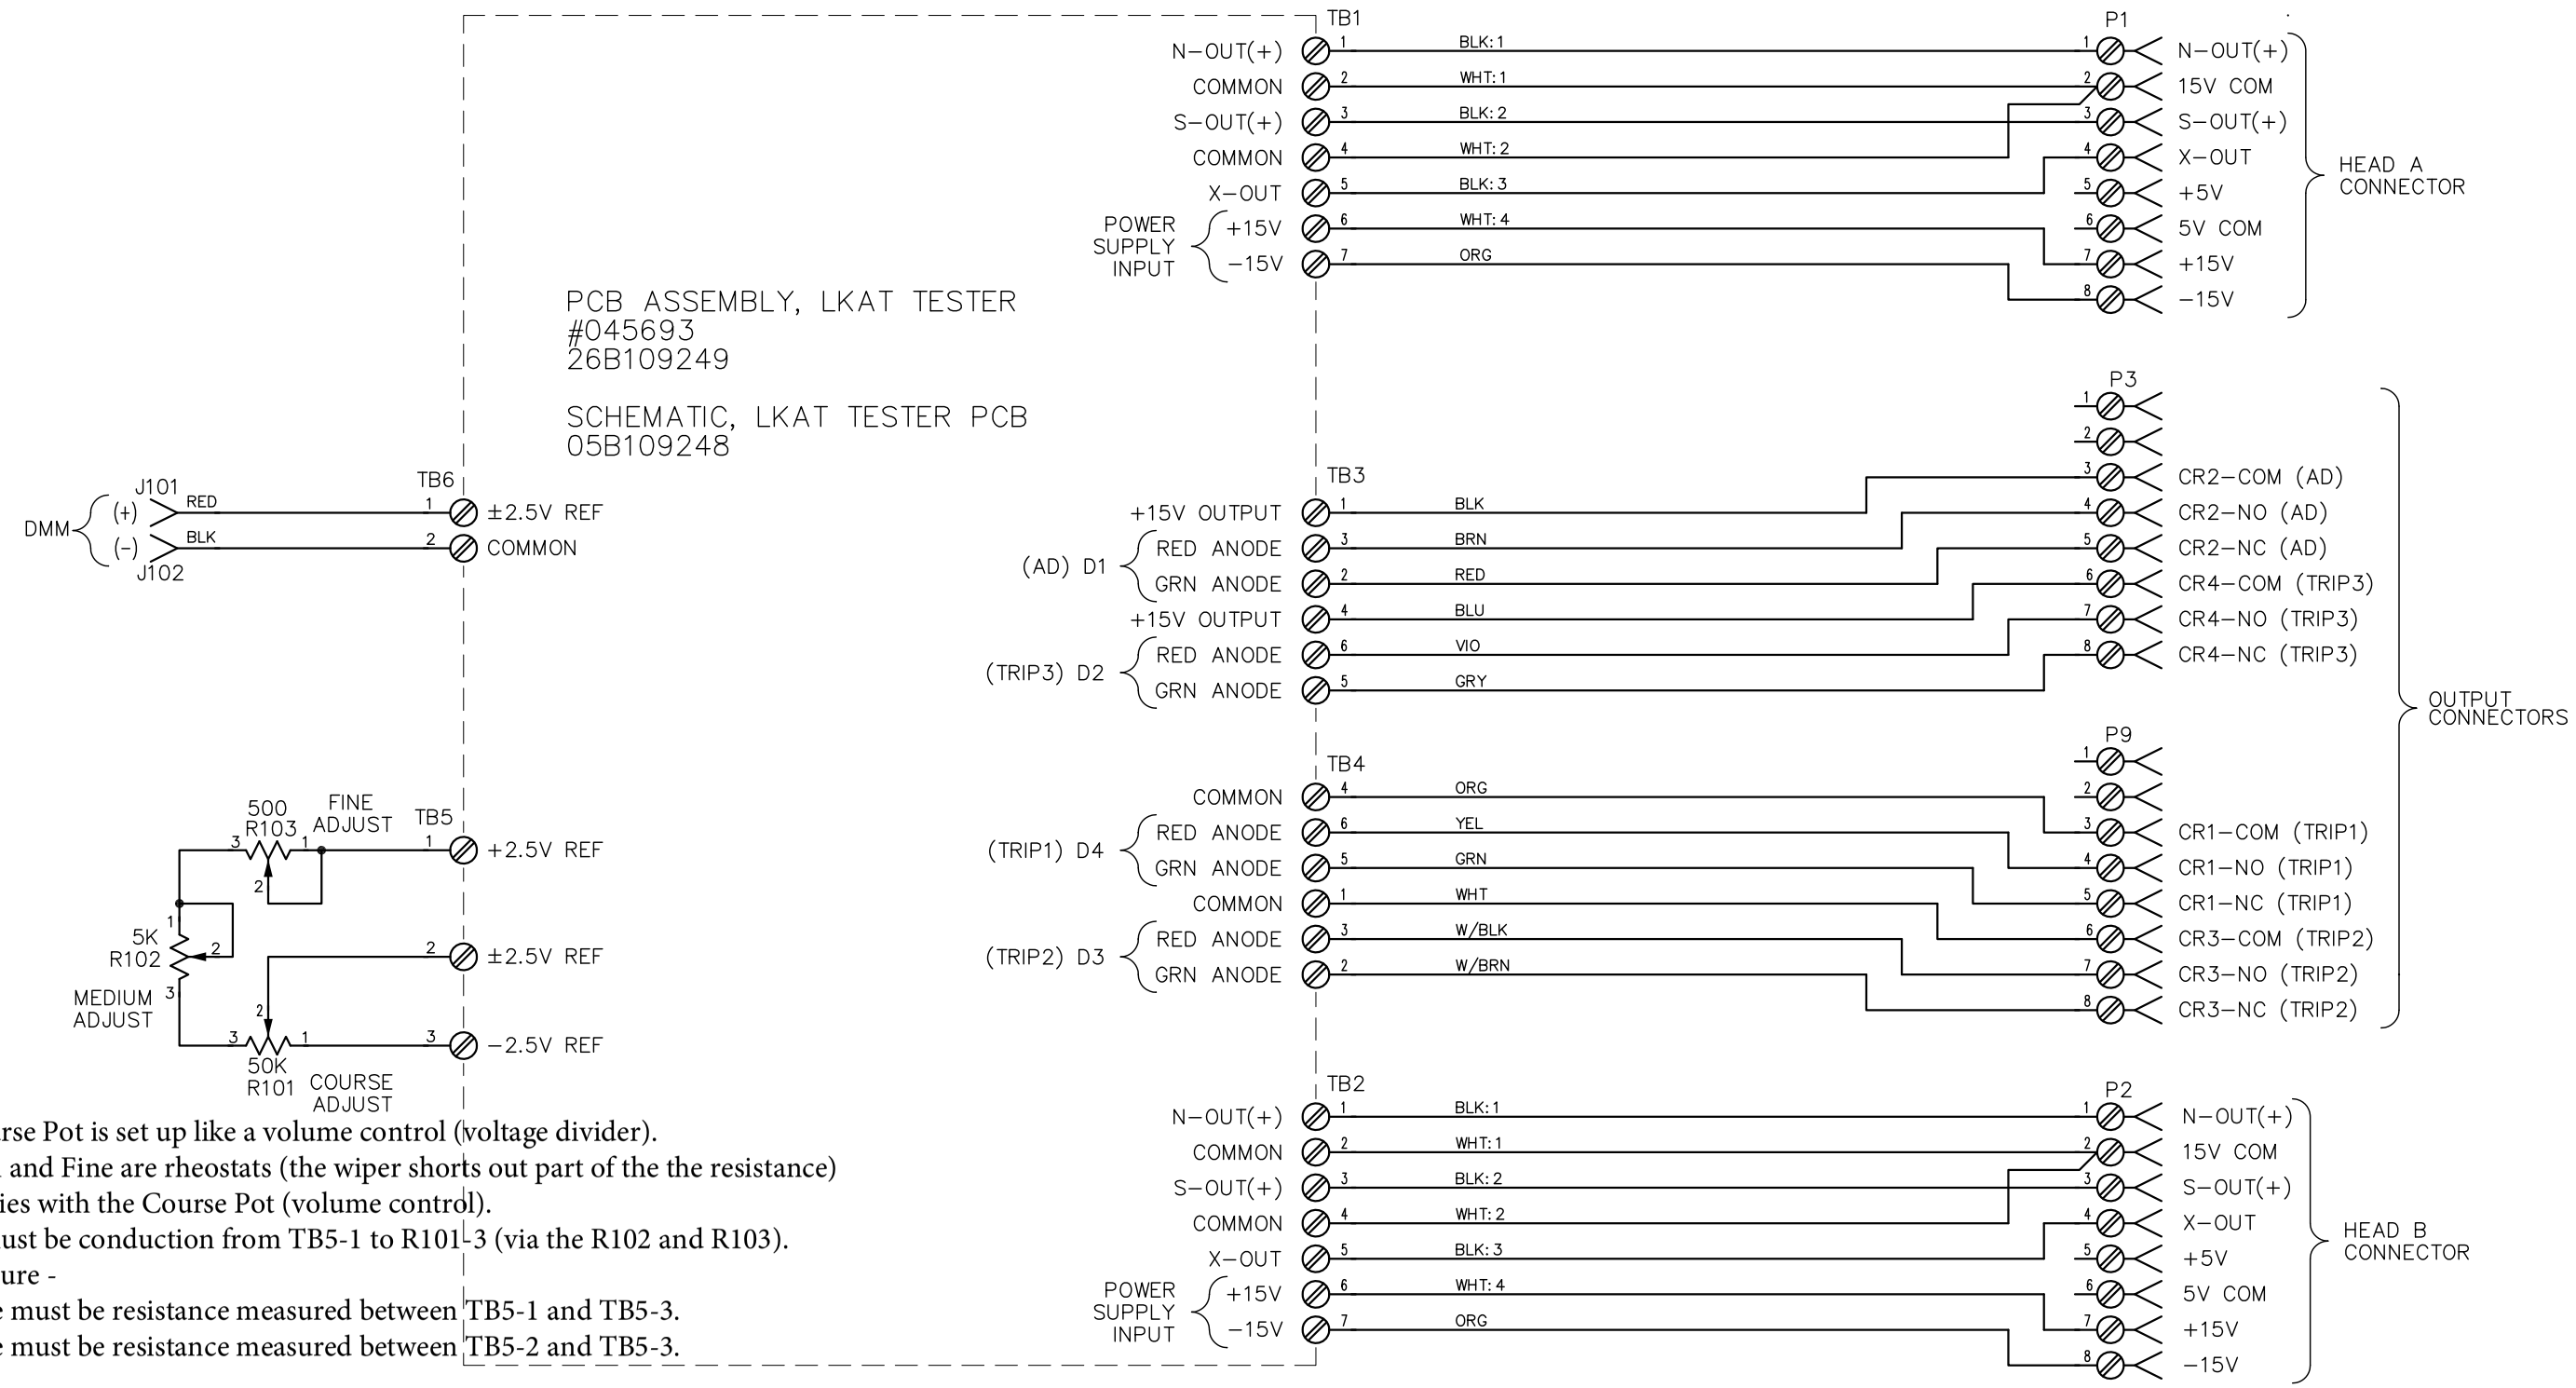

The Coarse Pot is set up like a volume control (voltage divider).
Medium and Fine are rheostats (the wiper shorts out part of the the resistance)
in series with the Course Pot (volume control).
There must be conduction from TB5-1 to R101-3 (via the R102 and R103).
To measure -
There must be resistance measured between TB5-1 and TB5-3.
There must be resistance measured between TB5-2 and TB5-3.

SYM.	REVISION	DRN./DATE	CK'S/DATE

THIS DRAWING AND ALL INFORMATION CONTAINED HEREIN, IS THE PROPERTY OF DynAmp LLC, AND MAY NOT BE COPIED, REPRODUCED NOR DIVULGED TO UNAUTHORIZED PERSONS WITHOUT THE EXPRESS WRITTEN CONSENT OF DynAmp LLC. IT IS PROVIDED SOLELY FOR THE CONVENIENCE OF THE USER AND SHALL BE RETURNED UPON REQUEST.

B/M NO.(REF.) 045709

THIRD ANGLE PROJECTION

DO NOT SCALE PRINT

TOL. UNLESS OTHERWISE NOTED: DEC. ±.015, FRAC. ±.015, ANG. ±1°

FINISH

MAT'L

DRN./DATE DEO 11/16/11

CK'D/DATE

SCALE N/A

APV./DATE

DynAmp, LLC GROVE CITY, OHIO

TITLE SCHEMATIC – LKAT SIGMA/OEM TESTER

JOB

DWG. NO. 05B109265

REV. –